


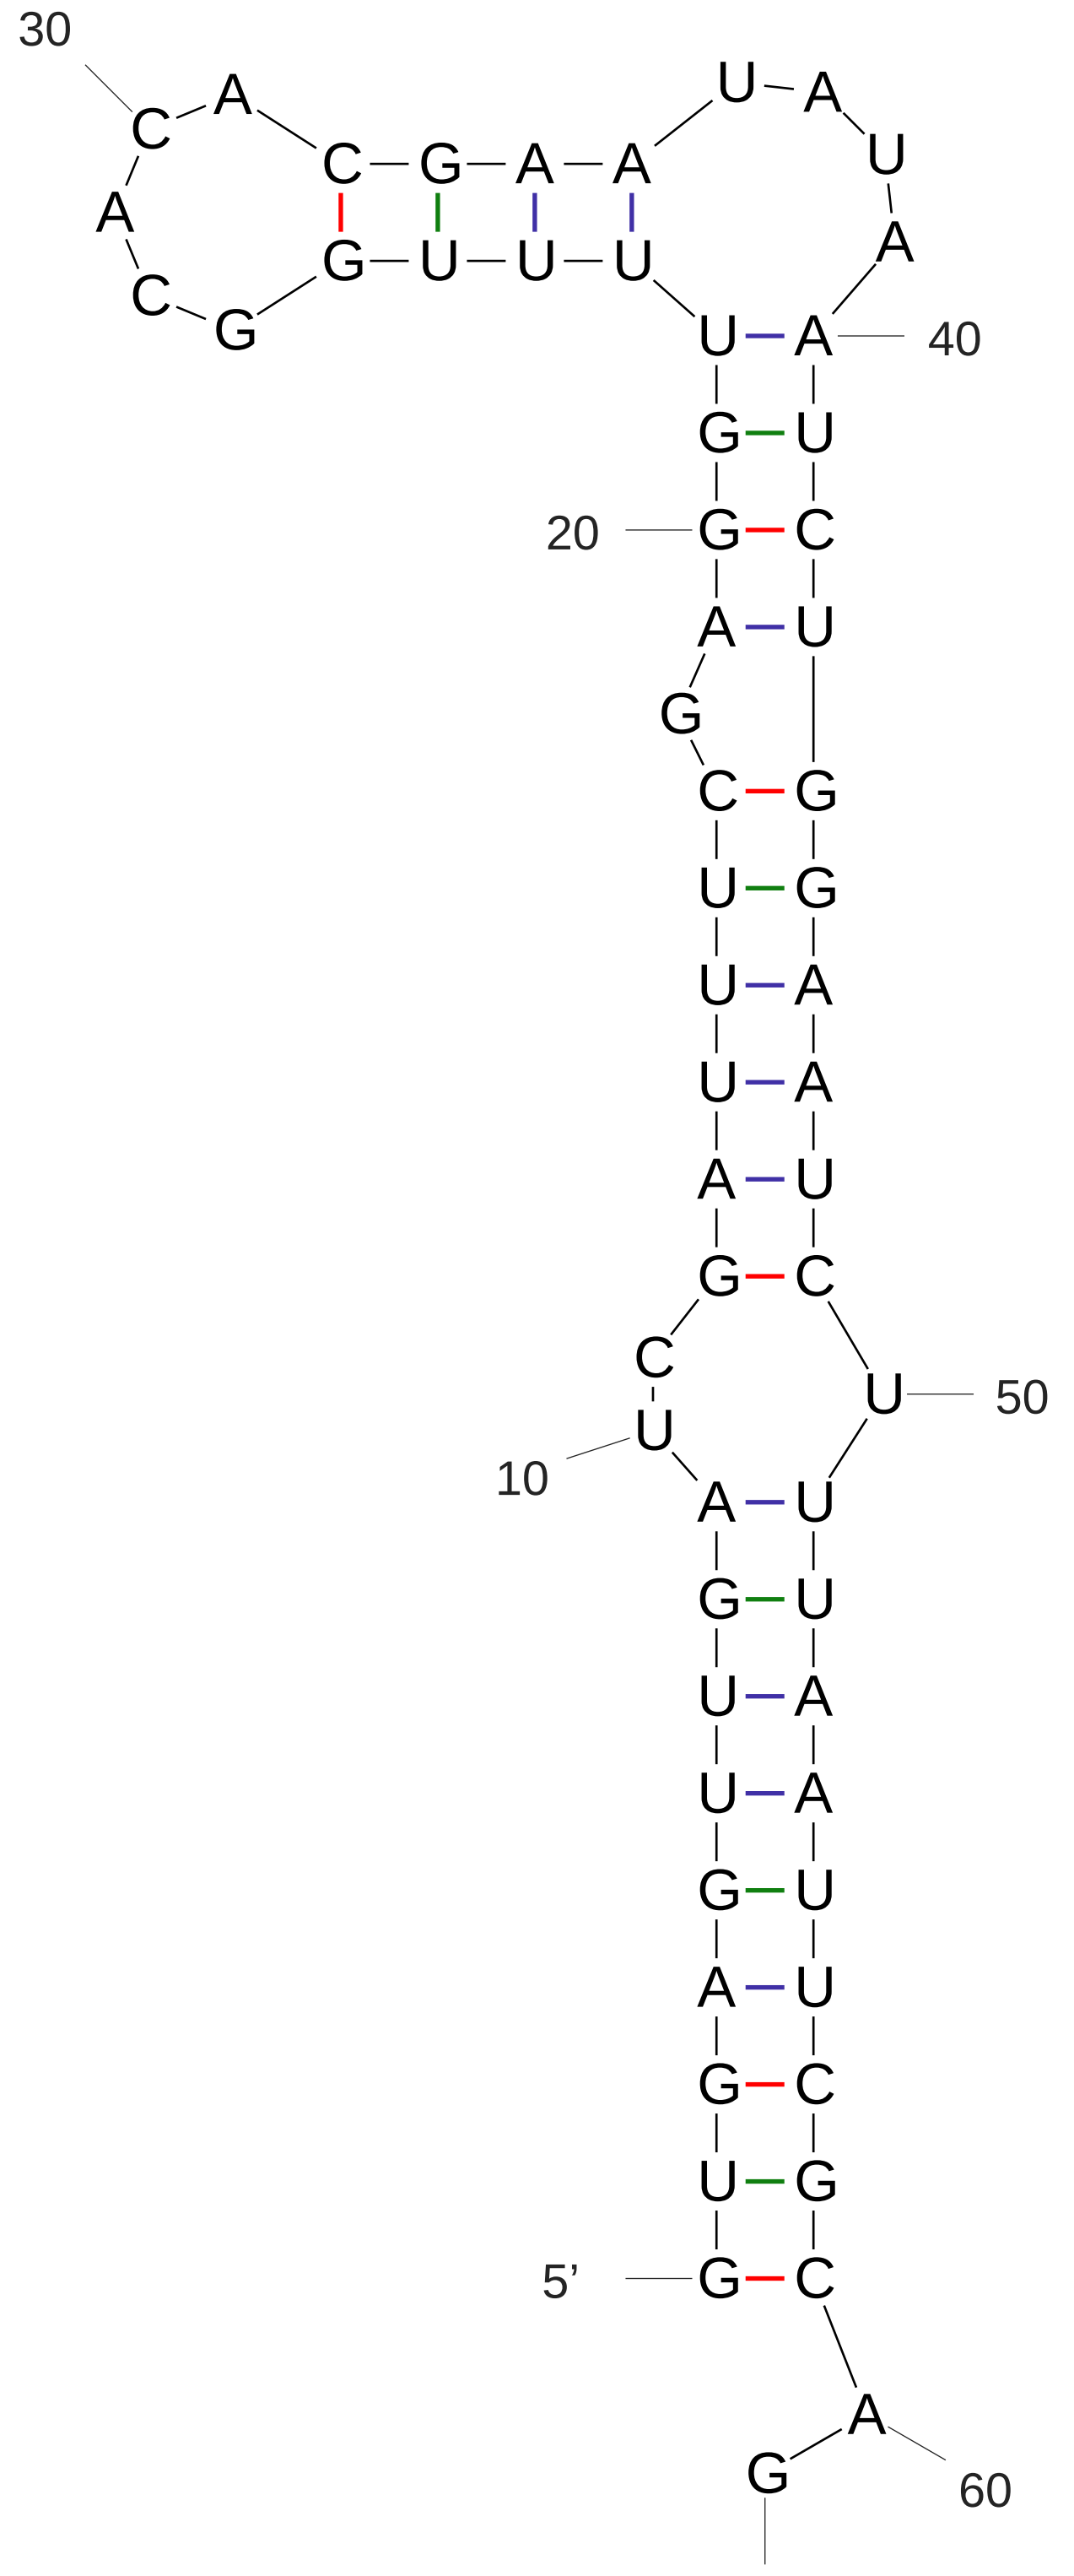

dG = -17.00 [Initially -17.00] dme-mir-1005 MI0005866